




Loading instruction - Viscoject Bio FEMTIS® Family with plate-haptic




FB-313



FB-313 MF15
FB-313 MF30



FB-313 MF15 TO-T3
FB-313 MF30 TO-T3

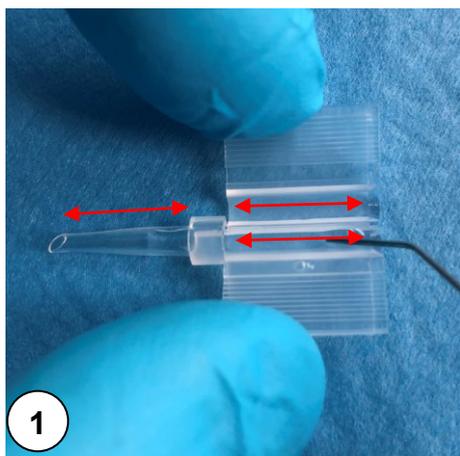

1

Lubricate the injector tip + loading chamber with viscoelastic solution.




2

Open the IOL blister away from your body.




3

Remove IOL holder, align handle towards your body. **Always keep it horizontal!**

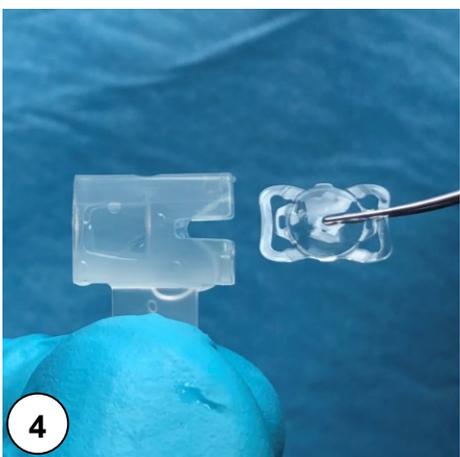


4

Notch should face to the right side! Remove the IOL from the holder with forceps without excessive force. **Use a non-toothed forceps!**

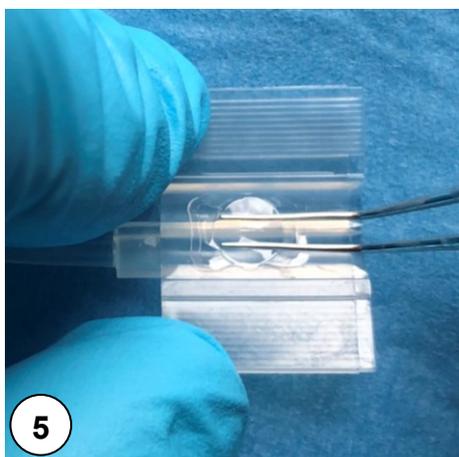

5

Place the IOL within the cartridge. Pay attention to marking A, B and C. Push the IOL down with forceps while closing the cartridge.

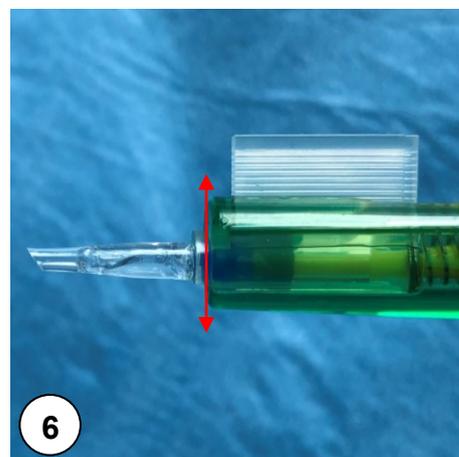

6

Place the cartridge into the injector. Push the plunger until the blue cushion reaches the tip, followed by short pressure relief. Implant the IOL.

